



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

DeLaLuna Alpaca/Dirk Busemann
Landwehr 115
44534 Lünen Germany

Date: 03/26/20

Test No: 987994


Animal and Sample Description

Animal Name: DLA Braveheart
Breed: Alpaca(Huacaya)
Sex: Male
Color: Brown

Animal ID: XXXXX
Sample Location: Side
Sample Date: 02/28/20
Age: 04/29/18

Laboratory Data

Mean Fiber Diameter:	21.5 microns	Fibers Greater Than 30 microns:	5.0 %
Standard Deviation:	4.8 microns	Comfort Factor:	95.0 %
Coefficient of Variation:	22.3 %	Mean Curvature:	32.3 deg/mm
Spin Fineness:	21.1 microns	SD Curvature:	20.8 deg/mm

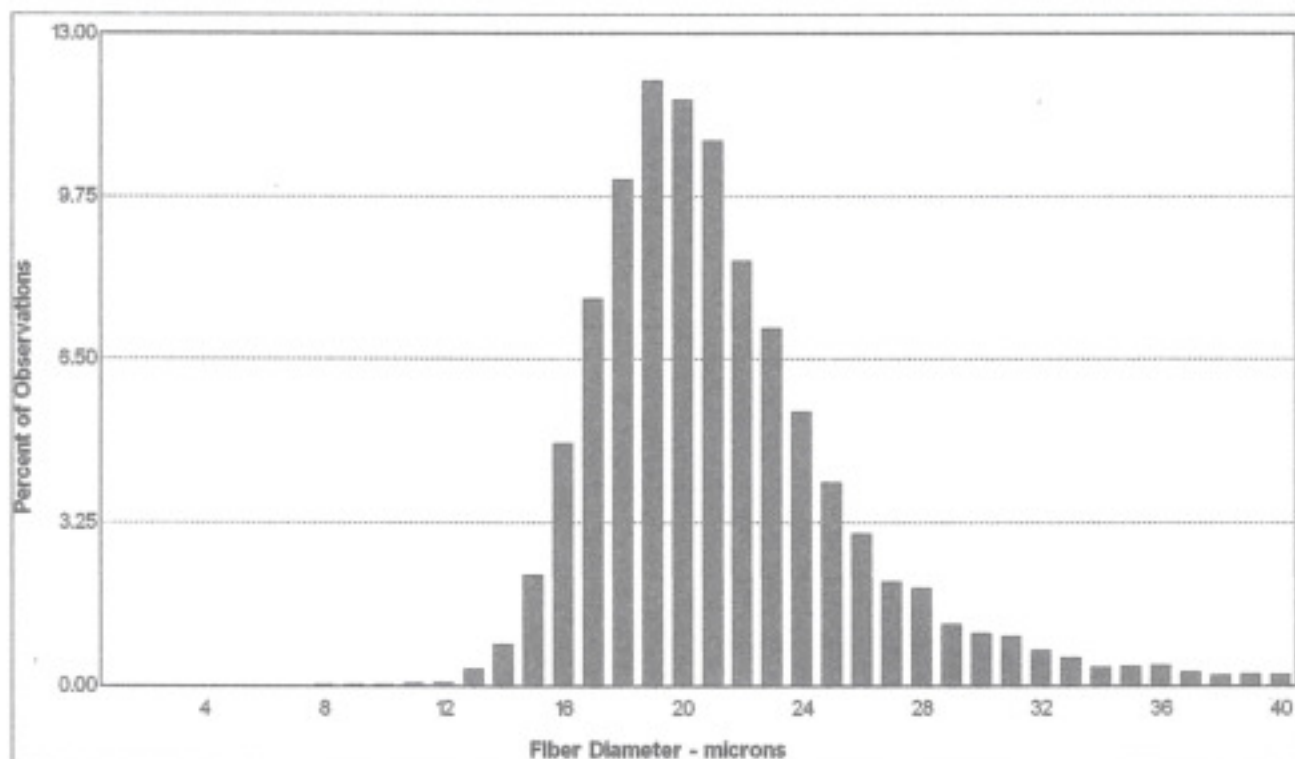

This Test Performed According to I.W.T.O Method 47