



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

DeLaLuna Alpaca/Dirk Busemann
Landwehr 115
44534 Lünen Germany

Date: 03/26/20

Test No: 987990


Animal and Sample Description

Animal Name: DLA Heartbreaker
Breed: Alpaca(Huacaya)
Sex: Male
Color: Lt Fawn

Animal ID: XXXXX
Sample Location: Side
Sample Date: 02/28/20
Age: 07/01/18

Laboratory Data

Mean Fiber Diameter:	16.6 microns	Fibers Greater Than 30 microns:	0.5 %
Standard Deviation:	4.2 microns	Comfort Factor:	99.5 %
Coefficient of Variation:	25.1 %	Mean Curvature:	40.0 deg/mm
Spin Fineness:	16.7 microns	SD Curvature:	23.4 deg/mm

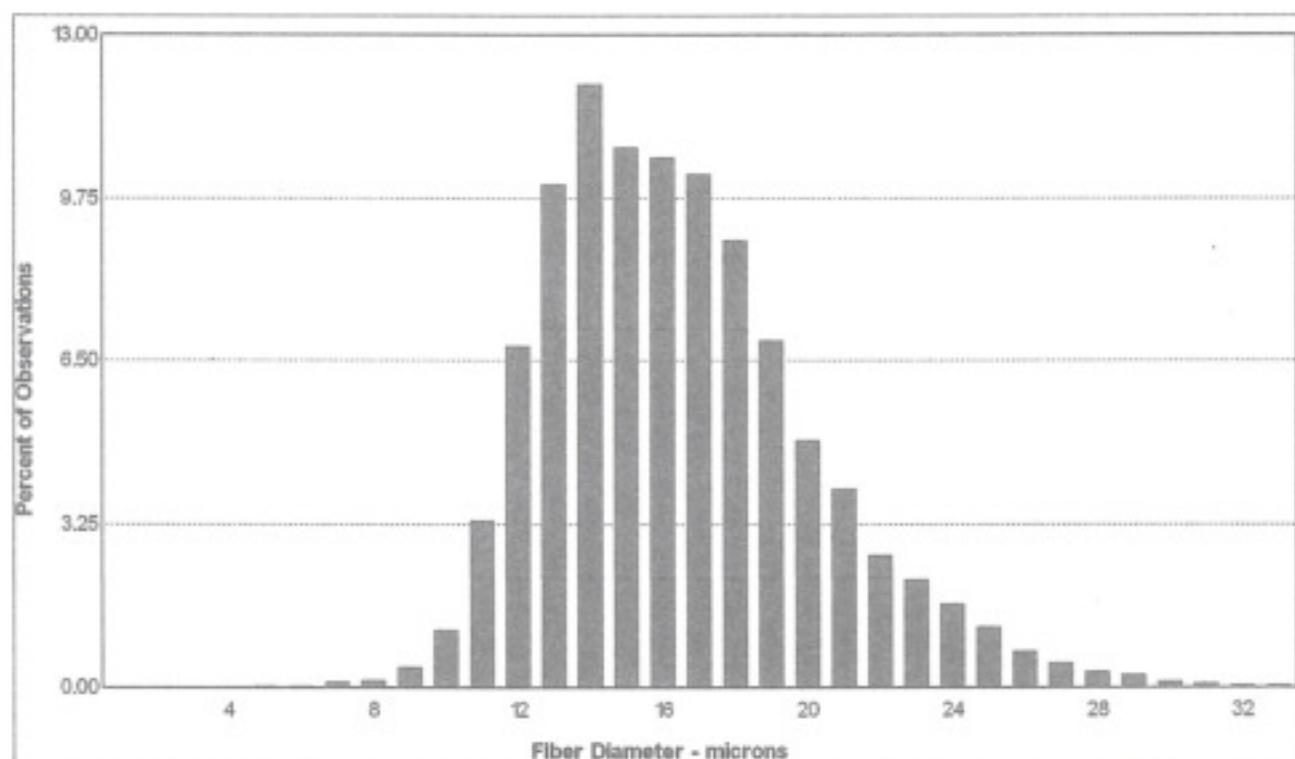

This Test Performed According to I.W.T.O Method 47